


TECNIS

Symphony[®]

Extended Range of Vision IOLs

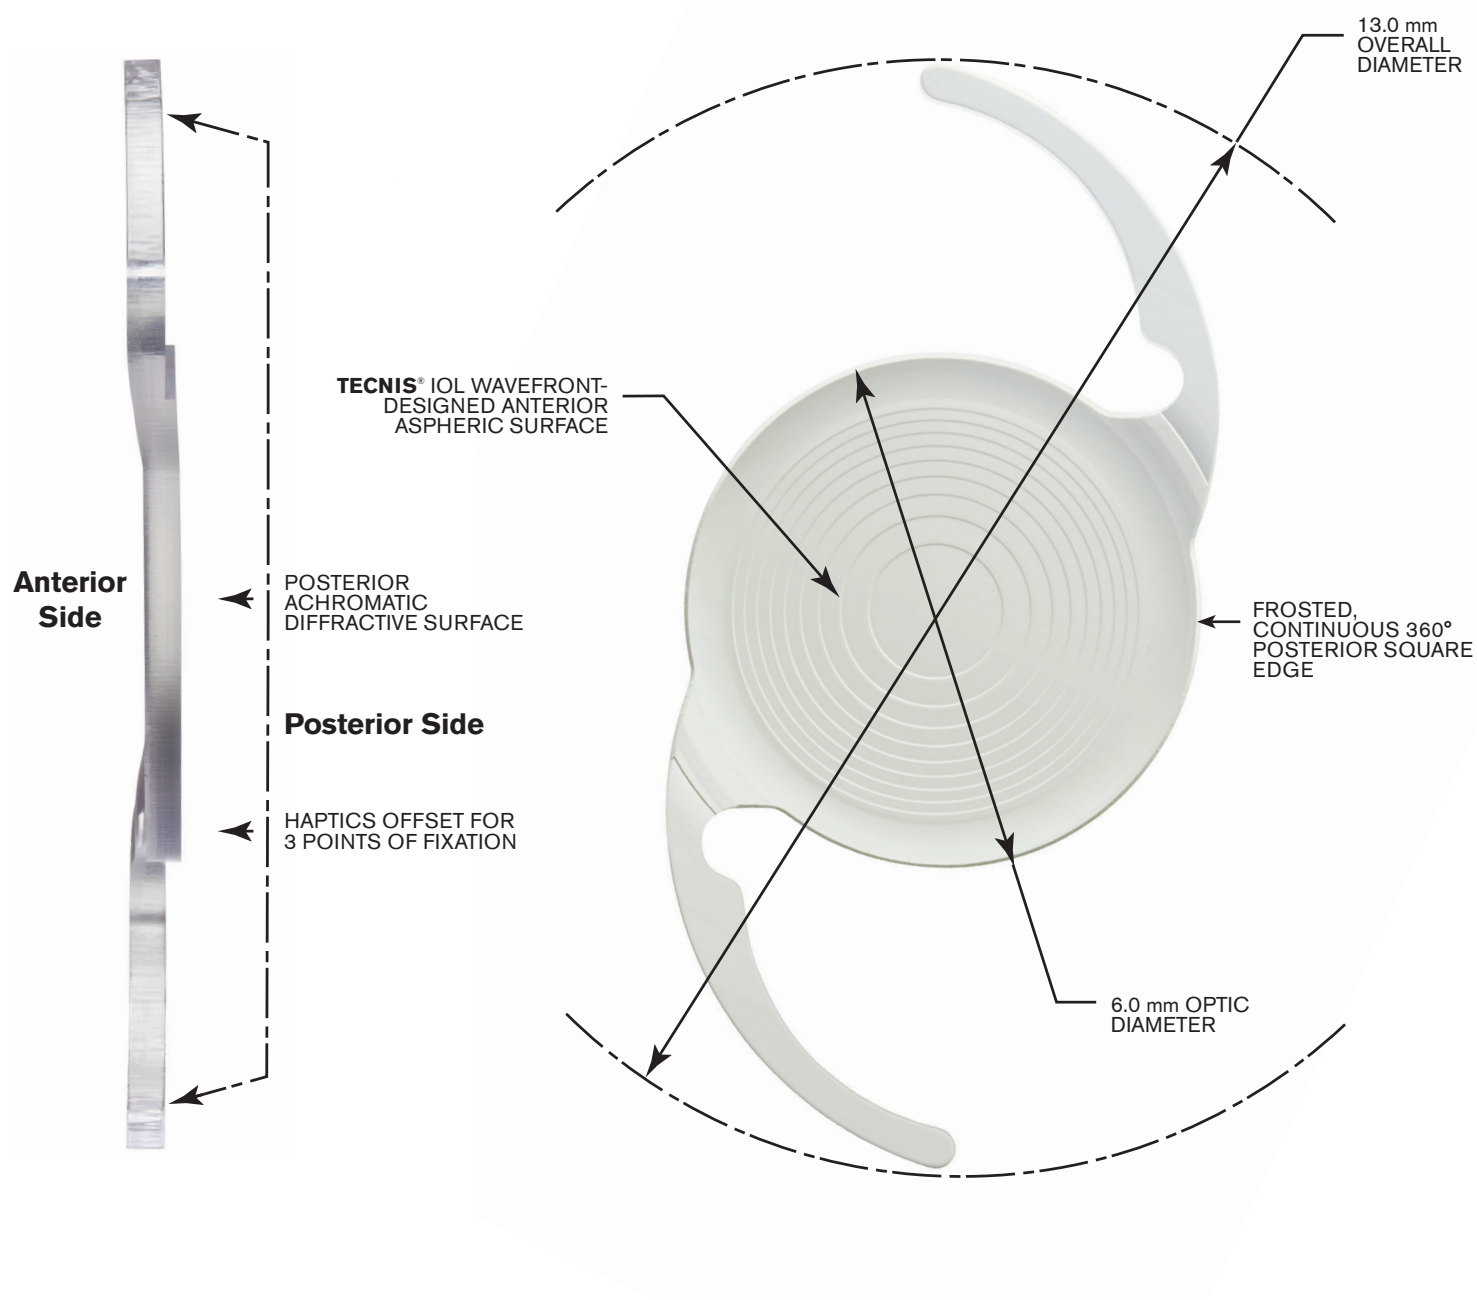

| DESCRIPTION | | |
|---|--|-----------------------------|
| OPTICAL CHARACTERISTICS | | |
| Powers: | +5.0 D to +34.0 D in 0.5 diopter increments | |
| Diameter: | 6.0 mm | |
| Center Thickness: | 0.7 mm (20.0D) | |
| Shape: | Biconvex, wavefront-designed anterior aspheric surface, posterior achromatic diffractive surface to enhance contrast sensitivity and echelette feature to extend the range of vision | |
| Material: | UV-blocking hydrophobic acrylic | |
| Refractive Index: | 1.47 at 35° C | |
| Edge Design: | ProTEC frosted, continuous 360° posterior square edge | |
| BIOMETRY* | CONTACT ULTRASOUND[†] | OPTICAL^{††} |
| A-constant: | 118.8D | 119.3D |
| AC Depth: | 5.4 mm | 5.7 mm |
| Surgeon Factor: [‡] | 1.68 mm | 1.96 mm |
| HAPTIC CHARACTERISTICS | | |
| Overall Diameter: | 13.0 mm | |
| Thickness: | 0.46 mm | |
| Style: | C | |
| Material: | Soft, Foldable, UV-blocking hydrophobic acrylic | |
| Design: | Tri-Fix , Haptics offset from optic; 1-piece lens | |
| RECOMMENDED INSERTION INSTRUMENTS | MODEL | |
| UNFOLDER [®] Platinum 1 Series Screw-Style Inserter | DK7796 | |
| UNFOLDER [®] Platinum 1 Series Cartridge | 1MTEC30 | |
| ONE SERIES Ultra Syringe-Style Inserter | DK7786 | |
| ONE SERIES Ultra Cartridge | 1VIPR30 | |

* Values theoretically derived for a typical 22.0 D lens. Johnson & Johnson Vision recommends that surgeons personalize their A-constant based on their surgical techniques and equipment, experience with the lens model and postoperative results.

[†] IOL constants have been theoretically derived for contact ultrasound.

^{††} IOL constants have been derived from clinical evaluation results of the 1-Piece IOL Platform.

1. Holladay JT. International Intraocular Lens & Implant Registry 2003. *J Cataract Refract Surg.* 2003; 29:176-197. REF2016CT0151.

TECNIS Symfony[®] Extended Range of Vision Lenses are indicated for primary implantation for the visual correction of aphakia in adult patients with and without presbyopia in whom a cataractous lens has been removed by extracapsular cataract extraction, and aphakia following refractive lensectomy in presbyopic adults, who desire useful vision over a continuous range of distances including far, intermediate and near, and increased spectacle independence. These devices are intended to be placed in the capsular bag. For a complete listing of precautions, warnings, and adverse events, refer to the package insert.

For healthcare professionals only.

Please read the Directions for Use for Important Safety Information and consult our specialists if you have any questions.

TECNIS, TECNIS SYMPHONY, ProTEC, TRI-FIX, UNFOLDER and ONE SERIES are trademarks of Johnson & Johnson Surgical Vision, Inc.

©Johnson & Johnson Surgical Vision, Inc. 2018

PP2018CT5142